

# Doppler 403™ & Mini-Doppler 1430™ Flow Phantoms

Reliable, Reproducible  
System Velocity Testing


- Collaboratively designed to better serve your needs
- Go from storage to use in less than 10 seconds



Verify ultrasound system and transducer performance. Doppler 403™ and Mini-Doppler 1430™ Flow Phantoms help assess system velocities using precision flow rates and proprietary blood-mimicking fluid.

Calibrating your Doppler ultrasound systems for accurate flow measurements optimizes the output, offering meaningful results to patients undergoing noninvasive testing.

- Precision pulsatile flow mode allows you to reliably test system velocities
- HE (High Equivalency) Gel™ is patented and proven
  - Helps ensure all transducers and system settings are fully tested across the entire frequency range from 2 to 18 MHz
  - Response of attenuation-to-frequencies over 8 MHz supports accurate axial resolution and penetration depth representative of human tissue<sup>1,2</sup>

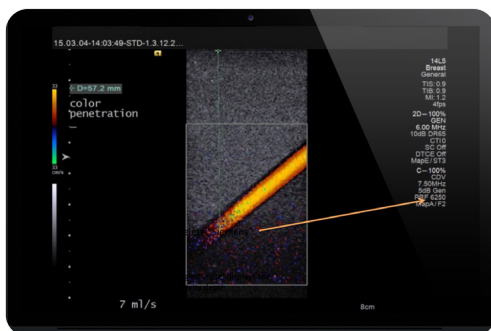

Scanning the angled vessel displays the color flow sensitivity depth.

<sup>1</sup> Browne, J., Ramnarine, K., Watson, A., Hoskins, P., Assessment of the Acoustic Properties of Common Tissue-mimicking Test Phantoms. Ultrasound in Medicine and Biology, Vol. 29 (7), pp. 1053-1060, 2003.

<sup>2</sup> Goldstein, A., The Effect of Acoustic Velocity on Phantom Measurements. Ultrasound in Medicine and Biology, Vol. 26, pp. 1133-1143, 2003.

<sup>3</sup> When combined with the flow controller

**sunnuclear.com**

7600 Discovery Drive, Middleton, WI 53562 USA

All data used is best available at time of publication. Data is subject to change without notice.

©2020 Gammex, a wholly owned subsidiary of Sun Nuclear Corporation. All Rights Reserved.

DopplerFlow\_113020

**PEO B.V.**

info@gotopeo.com  
www.gotopeo.com

**The Netherlands**

Havenweg 16, 6603 AS Wijchen  
+31 (0)24 648 86 88

**Belgium**

Watmolenstraat 2, B-2910 Essen  
+32 (0)3 309 32 09

**CoC 34107894**

**VAT NL807859151B01**

**IBAN NL29 RABO 0356 1960 46**


**BIC RABONL2U**



## From routine QA to education and complex research

### Doppler 403 Flow Phantom

- The reference standard in Doppler Ultrasound QA
- Laminar and parabolic flows are available (velocity dependent)
- Includes the Sono Transducer Holder
- New blood mimicking fluid formulation
- No need to ever purchase or store blood mimicking fluid
- Increased viscosity and decreased Reynolds number

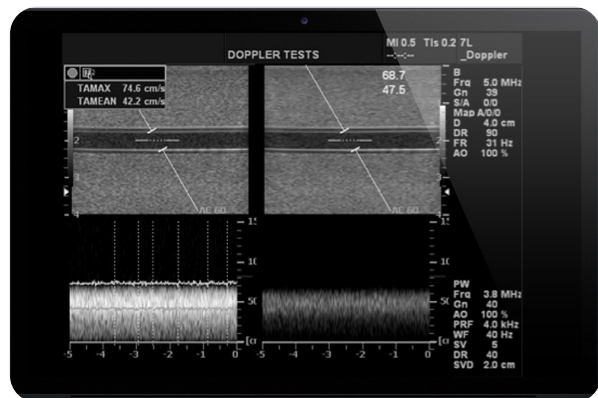

Volume flow settings on the phantom support reliable system velocity testing.

### Mini-Doppler 1430 Flow Phantom

- Ideal for cardiology and musculoskeletal (MSK) applications
- Portable and lightweight (<10 lbs / 4.6 kg)

### Common Highlights

- Patented multi-frequency HE Gel™
- Constant and pulsatile flow modes
- Rugged, self-contained, battery-operated

*"The tissue-like properties in Sun Nuclear ultrasound phantoms make them ideal for testing the performance of scanners."*

James A. Zagzebski, Ph.D., FAAPM  
Professor Emeritus, Retired Chair  
Department of Medical Physics,  
Wisconsin Institutes for Medical Research

### Sono Transducer Holder

The Sono Transducer Holder Accessory fits any Gammex phantom including the Sono Family and Doppler Flow phantoms.

- Place a transducer in a precise location in the holder for reproducible tests over time
- Support the transducer cable with the cable hook

### Sono Transducer Holder

Securely holds a transducer in a precise location to help you perform reproducible QC tests



[sunnuclear.com](http://sunnuclear.com)

7600 Discovery Drive, Middleton, WI 53562

PEO B.V.

[info@gotopeo.com](mailto:info@gotopeo.com)  
[www.gotopeo.com](http://www.gotopeo.com)

The Netherlands

Havenweg 16, 6603 AS Wijchen  
+31 (0)24 648 86 88

Belgium

Watermolenstraat 2, B-2910 Essen  
+32 (0)3 309 32 09

CoC 34107894


VAT NL807859151B01

IBAN NL29 RABO 0356 1960 46


BIC RABONL2U



## Precision pulsatile flow mode supports reliable system velocity testing

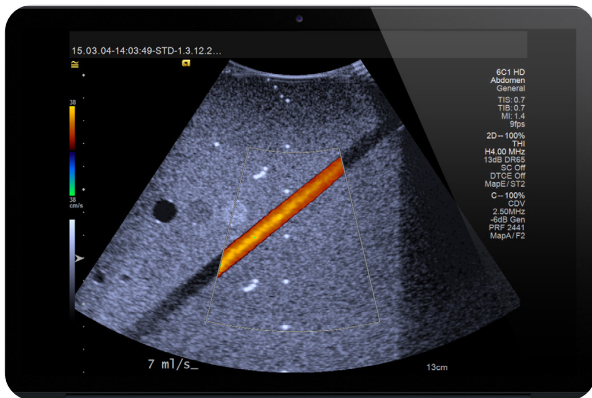

The Doppler 403 Flow Phantom is used to test the Doppler color flow velocity measurement.

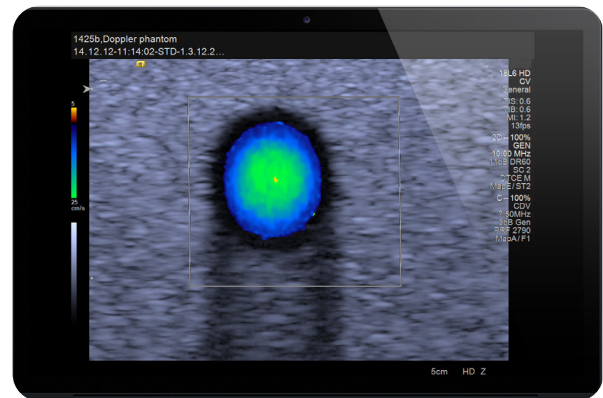

Cross section image showing the highest velocity at the center of the tubing. This represents a measurement of laminar, parabolic flow.

### Rejuvenation Will Protect Your Investment

Our Doppler Flow and Sono (B-Mode) phantoms are the only ultrasound phantoms on the market that can be rejuvenated and re-validated. Implementing a rejuvenation program can extend the life of the phantom to 10+ years.

**PHANTOM + REJUVENATION PROGRAM = 10 YEARS OF PHANTOM LIFE = CONSISTENT SYSTEM PERFORMANCE EVALUATION OVER TIME**

### Specifications

	Doppler 403 Flow Phantom	Mini-Doppler 1430 Flow Phantom
HE Gel™ Multi-Frequency Tissue-Mimicking Material	✓	✓
Patented Composite Film Scanning Surface	✓	✓
Vessels (2)	5 mm inner diameter; 1 horizontal at 2 cm depth, 1 diagonal at 40° from 2 to 16 cm deep	4mm inner diameter; 1 horizontal at 2 cm depth, 1 diagonal at 35° from 2 to 9 cm deep
Flow Rates	Customizable, constant and pulsatile	Customizable, constant and pulsatile
Blood Mimicking Fluid	Speed of Sound 1550 +/- 10 m/s	Speed of Sound 1550 +/- 10 m/s
Targets	Strings, cysts, grey scale, resolution groups	Strings, cysts, grey scale, resolution groups
Dimensions (Case)	28 H x 30.5 W x 22 cm D (11 x 12 x 8.65 in.)	20 H x 23 W x 15.2 cm D (7.87 x 9.06 x 5.94 in)
Weight	8.34 kg (18 lbs. 4 oz.)	4.6 kg (9 lbs. 15 oz.)