


Tissue Equivalent Ultrasound Prostate Phantom

Model 053S, 053L & 053L-EF

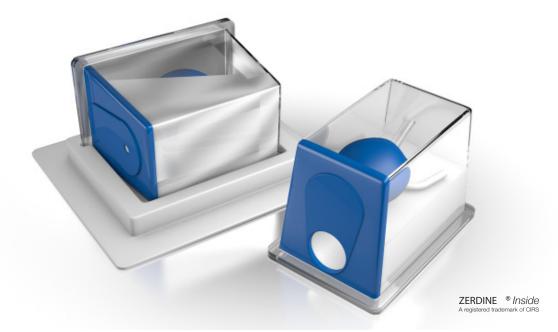

THE IDEAL TRAINING DEVICE FOR ULTRASOUND GUIDED PROCEDURES


The CIRS Ultrasound Prostate Training Phantom is a multimodality disposable phantom developed for practicing procedures which involve scanning the prostate with a rectal probe.

Gel formulations within the Model 053S, 053L and 053L-EF are designed to minimize needle tracking and to provide imaging contrast under CT, MRI, ultrasound and elastography.

The prostate along with structures simulating the rectal wall, seminal vesicles and urethra is contained within an $11.5 \times 7.0 \times 9.5$ cm clear acrylic container. A 3 mm simulated perineal membrane enables various probes and surgical tools to be inserted into the prostate. This phantom is an ideal training device for ultrasound guided cryosurgery, radioactive seed implantation, and needle biopsy.

The phantom is available with lesions (053L) and without lesions (053S) and can be ordered in either the standard side-fire configuration or an alternate geometry optimized for end-fire probes (053L-EF).





Features

- Includes rectal wall, seminal vesicles, perineal membrane and urethra
- Train for ultrasound-guided cryosurgery, seed implantation and needle biopsy with one phantom
- Compatible with various probes and surgical tools
- Structures visible under CT, MRI, ultrasound and elastography
- Gel designed to minimize needle tracking

900 Asbury Ave • Norfolk, Virginia 23513 • USA Tel: 800.617.1177 • 757.855.2765 • Fax: 757.857.0523

WWW.CIRSINC.COM



PEO B.V.

info@gotopeo.com www.gotopeo.com The Netherlands

Havenweg 16, 6603 AS Wijchen +31 (0)24 648 86 88 Belgium


Watermolenstraat 2, B-2910 Essen +32 (0)3 309 32 09 CoC 34107894 VAT NL807859151B01 **IBAN** NL29 RABO 0356 1960 46 **BIC** RABONL2U







TISSUE EQUIVALENT ULTRASOUND PROSTATE PHANTOM

Model 053S, 053L & 053L-EF

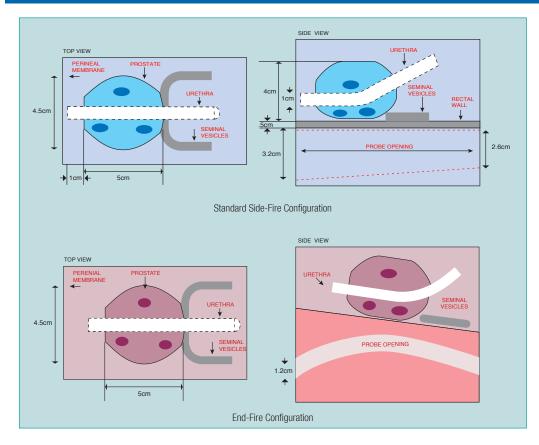





053L MR T1 Weighted

SPECIFICATIONS

CONTAINER

Dimensions: 11.5 x 7 x 9.5 cm Weight: 2 lbs Front probe opening: 3.2 cm Ø

Rear probe opening: 2.6 cm Ø

BACKGROUND GEL

Ultrasound appearance: anechoic

CT appearance: dark

MRI appearance: dark (T1 weighted) Elastography: soft

URETHRA

Dimensions: 7 mm Ø

Ultrasound appearance: anechoic

CT appearance: dark, similar to prostate MRI appearance: dark than prostate (T1 weighted) Elastography: stiffer than prostate

PROSTATE

Dimensions: 5 cm x 4.5 cm x 4 cm Ultrasound appearance: average echo-

ČT appearance: dark, slight contrast with

background

MRI appearance: bright (T1 weighted) Elastography: soft, slight contrast with

background Volume: 53 cc

SEMINAL VESICLES
Dimensions: 7 mm Ø x 10 cm long
Imaging appearance is similar to prostate

PERINEAL MEMBRANE

3 mm thick Z-skin™ elastomer

LESIONS (053L AND 053L-EF)

Qty: 3

Dimensions: Approximately 10 mm Ø Ultrasound appearance: hypoechoic CT appearance: bright

MRI appearance: dark (T1 weighted) Elastography: stiff

RECTAL WALL

Dimensions: 6 cm x 11 cm x 0.5 cm Imaging appearance is similar to urethra

MODEL 053 INCLUDES
Tissue Equivalent Ultrasound
Prostate Phantom

User Guide 12-Month Warranty* *Please note: once any device has been inserted into the phantom (such as biopsy needles, localization wires, etc.) the 12 month warranty will not cover claims related to material desiccation or needle

(1) US Patent # 5196343

PROSTATE PHANTOM SELECTION GUIDE

Model	Description	Transducer Type
053S	Prostate Phantom without Lesions	Side-Fire or BiPlane
053L	Prostate Phantom with Lesions	Side-Fire or BiPlane
053L-EF	Prostate Phantom with Lesions for End-Fire Transducer	End-Fire Transducer

 $^{\circ}2013$ Computerized Imaging Reference Systems, Inc. All rights reserved. Specifications subject to change without notice. Publication: 053S 053L 053LEF DS 062421



ComputerizedImagingReferenceSystems,Inc.hasbeencertifiedbyULDQS Inc. to (ISO) 13485:2016. Certificate Registration No.10000905-MP2016.



info@gotopeo.com

www.gotopeo.com

+32 (0)3 309 32 09